

New Zealand Sports Turf Institute

Laboratory Analysis Test Results

Sample Details


Origin of Sample: McCallum Bros
 Sample Name: Turf Chip
 Date Received: 28.7.21
 Date Tested: 28.7.21

Particle Size Distribution - Drainage Gravel

Category	Diameter (mm)	Dry Weight (g)	Percent in Category
V. Coarse Gravel	8 - 16	0.0	0.0
Coarse Gravel	4 - 8	460.0	88.9
Fine Gravel	2 - 4	53.7	10.4
V. Coarse Sand	1 - 2	1.6	0.3
Sand, Silt & Clay	<1	2.1	0.4
Total		517.3	100.0

Result

Sieve Size	Percent Passing	Specification (min - max)
16.0	100.0	100
8.0	100.0	98 - 100
4.0	11.1	15 - 40
2.0	0.7	0 - 2
1.0	0.4	0 - 1

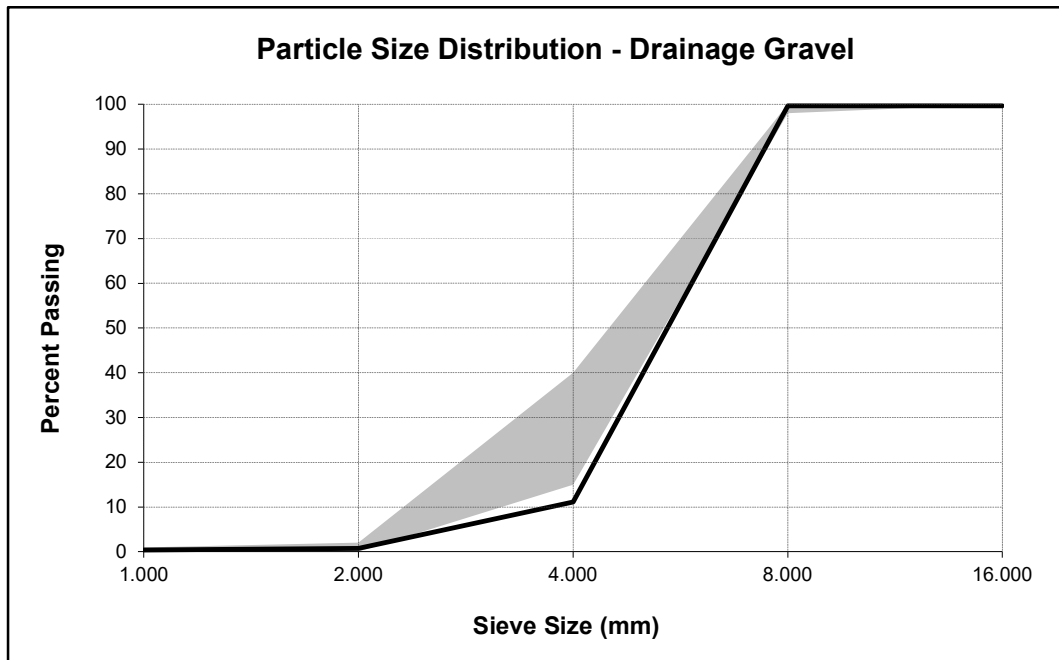

Checked by:



Brendan Hannan

Date:

28 July 2021